altosa®
SFT | ALTOSA SFT BALLOON CATHETER

compliance in tacking peripheral stent grafts

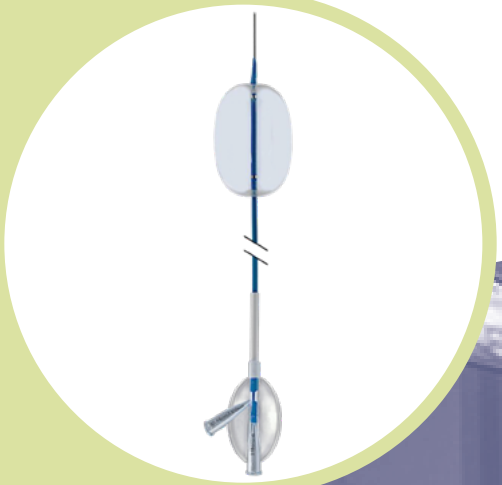

andratec®
ADVANCED INTERVENTIONAL TECHNOLOGIES

altosa® SFT
ALTOSA SFT BALLOON CATHETER

- Especially designed for large lumen dilatation and/or tacking of peripheral endoprosthesis.
- Enhanced inflation/deflation times for safe and easy use.
- Highly puncture resistant and reliable Polyurethane balloon material for multiple dilatations.
- Enhanced visibility prioviding higher accuracy in positioning.
- Low profile offering easy advancement through small introducers sheaths / delivery systems.
- Combines perfectly with state-of -the-art stent-grafts.



Technical Information

Balloon Material	Polyurethane Material
Balloon Compliance	Compliant
Shaft Diameter	10.5 F
Balloon Marker Distance	40 mm
Recommended max Diameter	46 mm
Balloon Length	46 mm
Rated Burst	50 mm at 100 ml
Shaft Length	65 cm / 100 cm
Recommended Guide Wire	0.035" (0.89 mm)
Recommended Sheath Introducer	12F

!! We recommend the use of an extra stiff guide wire such as the Lokum 'L-Quest' Guide Wire or the Lokum 'Amplatz-Type' Guide Wire.

Sizing Oriented Filling Volume

∅ (mm)	10	20	25	30	35	40	46
(ml)	2	9	15	25	35	45	65

Filling Volume Oriented Sizing

(ml)	5	10	20	30	40	50	65
∅ (mm)	15	18	27	33	38	42	46

Order Codes

A choice of various diameters and lengths.

Product Code	∅ (mm)	⟷ (mm)	↕ (cm)	(inch)
AL-46-65	46	46	65	0.035"
AL-46-100	46	46	100	0.035"

andratec® ADVANCED INTERVENTIONAL TECHNOLOGIES

andratec gmbh
Simmerner Straße. 70, 56075 Koblenz, Germany

Office & Warehouse
Im Deutschen Kaiser,
Kastorstraße 3, 56068 Koblenz, Germany
+49(0) 261 100 49 653
+49(0) 261 100 49 654
info@andratec.com

www.andratec.com

alliance partner

DEVELOPED IN GERMANY • MADE IN EUROPE •

CE 0123

∅ Balloon diameter (mm) (ml) Filling Volume (ml) ⟷ Balloon lenght (mm) ↕ Shaft Length (cm) Max. Rec. Guide Wire Size (")

2026/05/01/P009/Rev 2E/Brochure